
# Figure 1



Creation of a reference file

Measuring and identifying an unknown sample

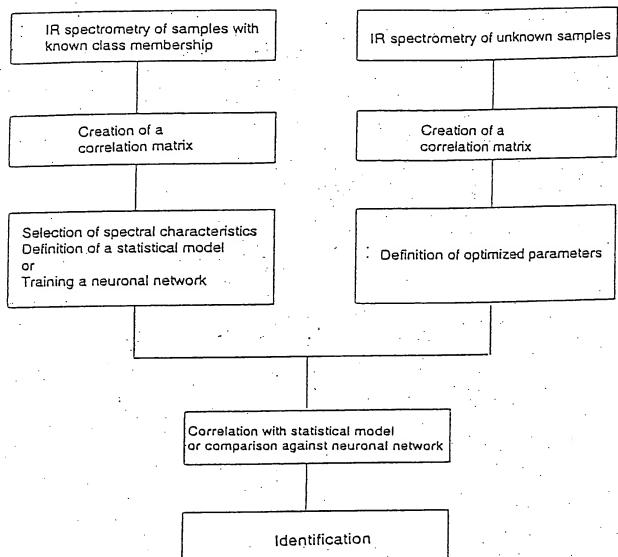

1000


1050

1100

1150

Wave number (cm<sup>-1</sup>)

1200

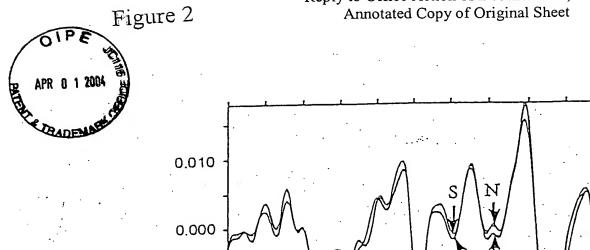

1250

Absorption

-0.010

-0.020

-0.030

- 1300

Figure 3



图]

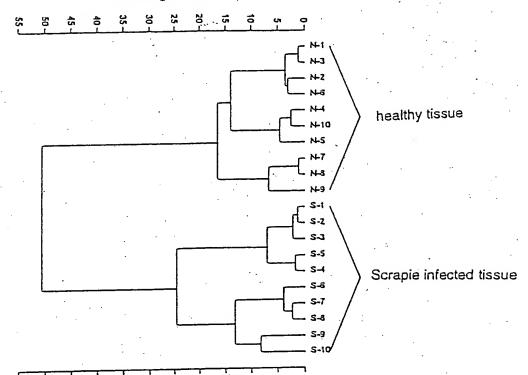


Figure 4A




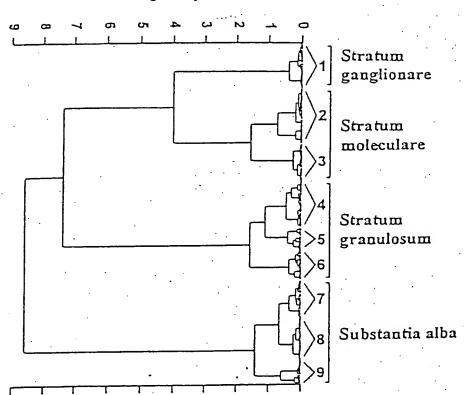


Figure 4B

APR 0 1 2004 A





# Figure 1

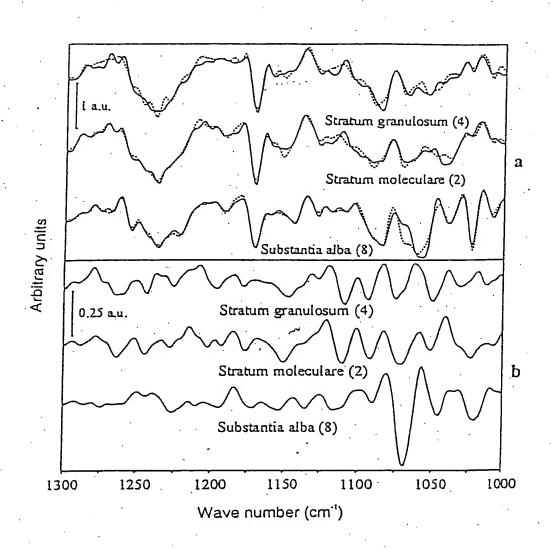

Creation of a reference file

Measuring and identifying an unknown sample

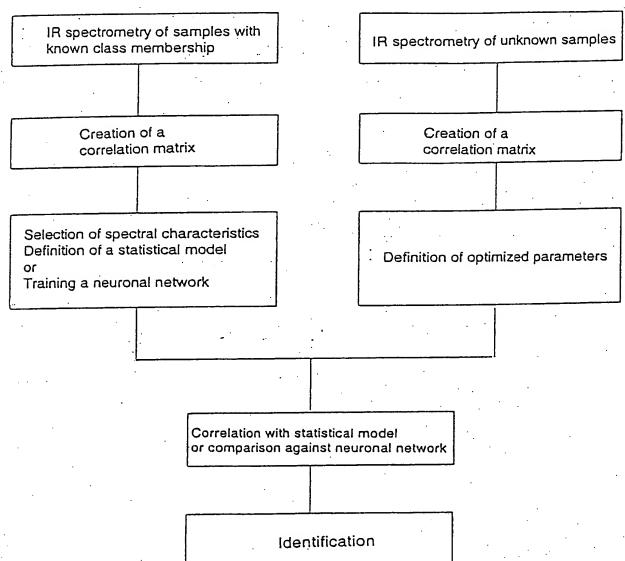



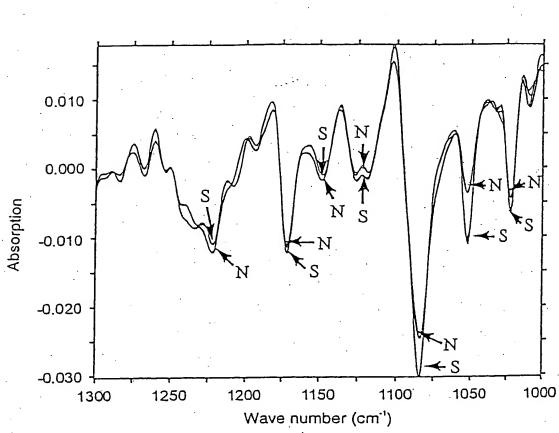


Figure 3



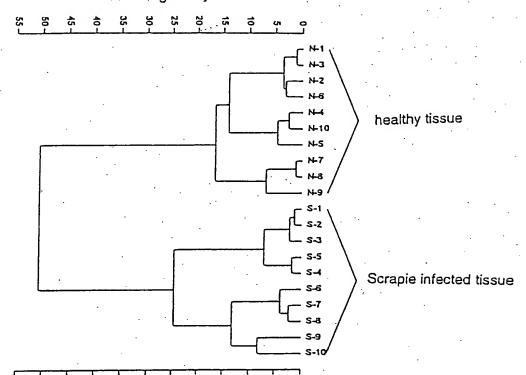


Figure 4A



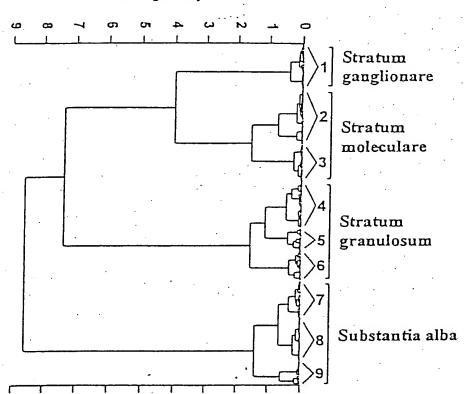


Figure 4B



